
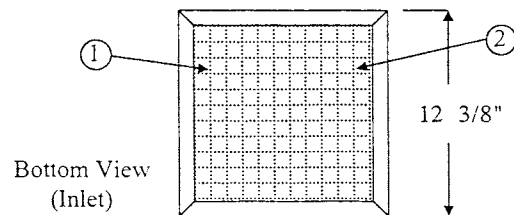
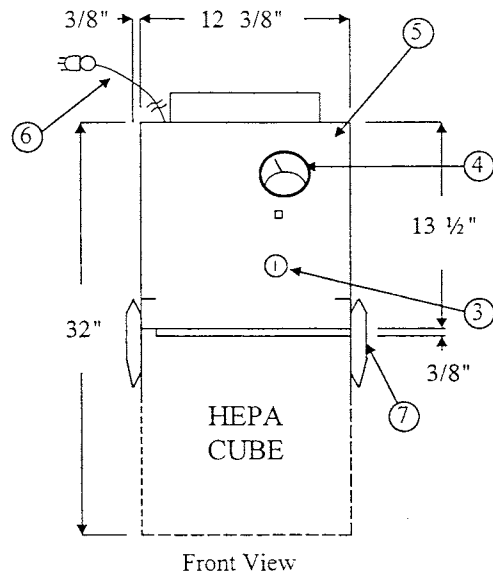
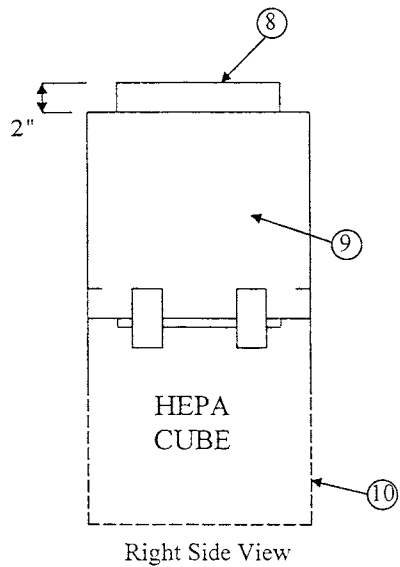


<b>BIOLOGICAL</b> <i>Controls</i>
SUBMITTAL DRAWING
Vertical Exhaust Module

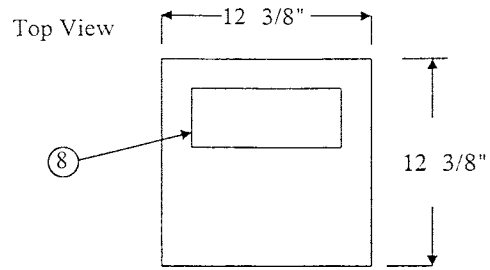

- (1) INLET GRILLE
  - (2) 1 EA. 1" TWO-PLY POLYESTER SYNTHETIC 35% EFFICIENT PRE-FILTER PANEL
  - (3) HIGH / OFF / LOW - KEY SWITCH
  - (4) 1 EA. MINIHELIC STATIC PRESSURE GAUGE
  - (5) 1 - BLOWER, PSC FORWARD CURVED, 1/5 HP, 115V - 50/60 Hz, TWO SPEED, 3.2A (HIGH) 2.07A (LOW) THERMAL RESET PROTECTED, AIRFLOW 495 HIGH, 435 LOW
  - (6) 1 EA. SIX (6) FOOT CORD, 18/3 CORD WITH 115V HOSPITAL GRADE PLUG
  - (7) 4 EA. HEPA FILTER CUBE DRAW LATCHES
  - (8) EXHAUST DUCT (6 X 9.875")
  - (9) UNIT CONSTRUCTED OF 20 GA. STAINLESS TYPE 304, #4 FINISH
  - (10) 1 EA. 12 X 12 X 11.5" HIGH CAPACITY HEPA FILTER RATED 99.99% ON 0.3 MICRON SIZE PARTICLES
- WEIGHT 34 #

Notes:  
ELECTRICAL REQUIREMENTS: 115V, 1 ph, 60 Hz., 1.0 FLA, 5 AMP FUSE,  
ELECTRICAL WIRING IS IN ACCORDANCE WITH THE LATEST NEC STANDARDS

Optional: HOUR METER

DRAWN FOR		<b>BIOLOGICAL</b> 749 Hope Road <i>Controls</i> Suite A Eatontown, NJ 07724			
STANDARD					TITLE MICROCON EX-BB-VE (top)
DRAWN BY	LVB	SIZE	JOB NO.	DWG NO.	REV
APPROVED BY		SCALE	1 1/2" = 1'-0"	DATE	July 15, 2002 SHEET